


Equipment for Enantioselective Liquid Chromatography

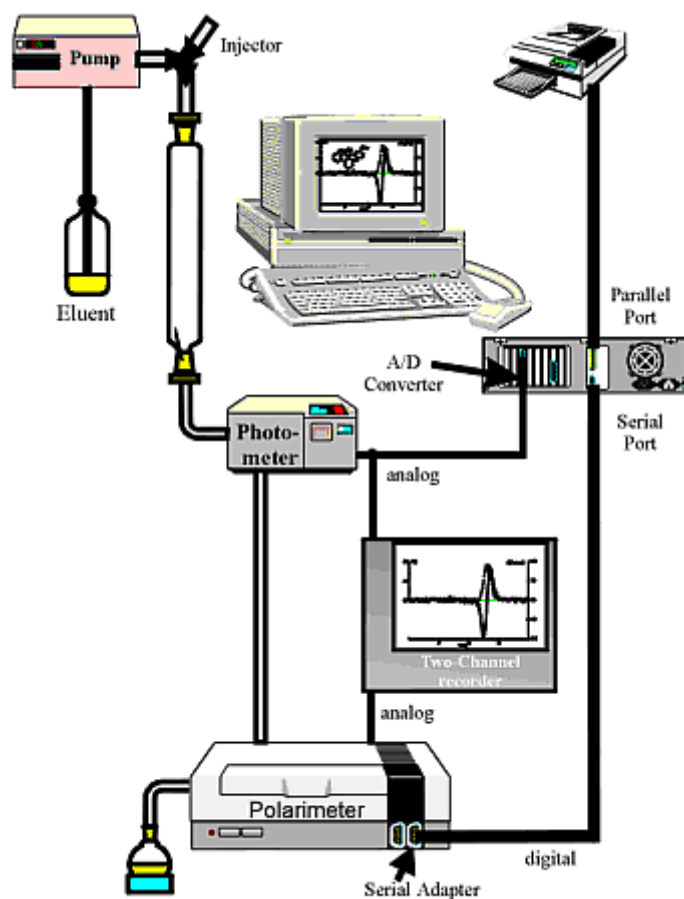

- Simultaneous collection, processing and plotting of the time-dependent data from two detectors (photometer and polarimeter or circular dichrograph) are performed by Windows software (M. Schinabeck, N. Costantini, H. Kopp).
- In particular, the deconvolution of overlapped peaks results in the optical purity of samples.
- See references 3, 4, 9 and 15 (Menu “Puplications”).